


# Oval Gear Flowmeter



- OG1
- OG2
- OG3
- OG4
- OG5
- OG6
- OG7
- Aluminium
- Stainless steel
- PEEK™
- Flanged or screwed
- Reed switch
- Hall effect
- IS Sensor option

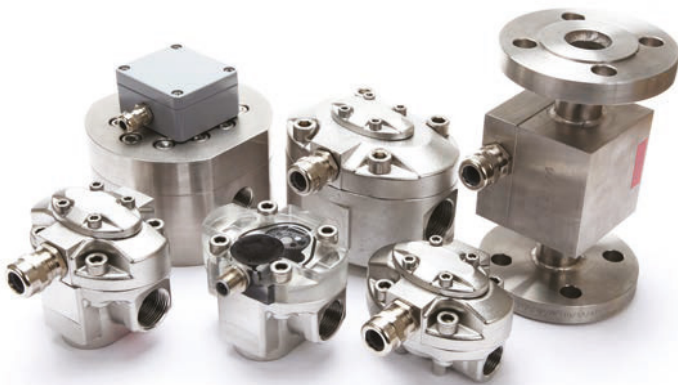

## INSTALLATION

The pipe-work should be designed in such a way to eliminate reverse flow. The meter should be installed in a position that prevents it from draining down as on start-up serious damage could result by “impacting” an empty flowmeter with a high velocity fluid stream. The fluid should be clean and homogenous. In all cases an upstream filter of at least 80 microns **MUST** be fitted.

**It is recommended that before the flowmeter is installed in the line a “dummy” section of pipe is inserted and the system flushed.** This is to eliminate any debris in that section of the line. The pipe must not stress the body of the meter and should be fully supported either side with appropriate isolation valves and in some cases a by-pass valve. On initial start-up increase the flow slowly to ensure no over speeding of the meter occurs as the air is forced from the line. This is best achieved by monitoring the flow rate and ensuring that a 50% over-range is not exceeded. **Never blow a flowmeter with an airline.** Care should be taken to ensure that no air enters the system (e.g. leaky pump gland) or that no cavitation takes place.

Oval gear flowmeters work by using the low differential pressure generated across the body to drive a pair of oval gears. This rotation can be detected by a variety of means to give either a TTL (NPN transistor) or contact closure pulse output. The unit is manufactured in a choice of materials and pressure ratings to suit most applications and as with all positive displacement flowmeters, the performance improves with increasing viscosity achieving an accuracy of  $\pm 0.1\%$  of reading with higher viscosities. The standard meters can be used up to 1000 cP; above this viscosity specially profiled gears **MUST** be used.

# Oval Gear Flowmeter



Distributor: DDM GmbH & Co. KG

Phone: +49 661 967 962-0 >>> Email: [info@ddm-sensors.de](mailto:info@ddm-sensors.de) >>> Web: [www.ddm-sensors.de](http://www.ddm-sensors.de)



## ELECTRICAL CHARACTERISTICS

Hall effect sensor		Reed switch	
Supply	8 to 24Vdc	Contact material	Rhodium
Temp range	-40 to 150°C	Voltage	24Vdc max
Rise and fall times	1.5µs max	Current	100mA max
Supply current	7.5mA typ	Operations	10 <sup>9</sup>
Switch current	10mA max	<i>'R' Series resistor 560Ω. For hazardous areas 'X' no protection is fitted.</i>	
Leakage current	10µA max		

It is recommended that all "signal" cables are screened and run separately to power lines and switched inductive loads and are located well away from inverters and other "noisy" apparatus. Always use sound wiring practice. Hall effect detector (**NPN**) requires an external pull-up resistor connected between the output and a suitable power supply to attain a pulse. Typically the flowmeter PSU may be used but sometimes a dc pulse, which is of a different voltage, may be required e.g. using a PLC with a 24V PSU and an internal 5V rail for the pull-up resistor/pulse input. The reed switch has a protection resistor of 560 Ohms in series with the connections unless it is specified for hazardous areas when the resistor is excluded.

## Connection options

M12 connector	Reed	Hall effect
Wireable plug 	Pin 3  Pin 4	Pin 1 +4.5-24V Pin 2 Not used Pin 3 0 Volts Pin 4 Output
Moulded plug 	White Not used Blue Black Brown Not used	Blue 0 Volts Brown +4.5-24V Black Output White Not used
Connector 	0V OP +V Not used	0V 0 Volts +V +4.5-24V OP Output
MIL socket 	Pin A Pin C Pin B Not used	Pin A 0 Volts Pin B +4.5-24V Pin C Output
Flying lead 	Screen Blue Red Not used	Screen 0 Volts Red +4.5-24V Blu Output




## COMMISSIONING

If problems occur during commissioning always check the fundamentals first.

- Is the flowmeter/instrument the correct one for the installation?
- Is the power connected to the meter and the instrument, and is it turned on?
- Is the instrument set/wired correctly? I/P port, pulse type, frequency span, units etc.
- Where possible check the O/P from the flowmeter with an oscilloscope before proceeding.
- Was the line flushed prior to installing the meter?
- Was the flow increased slowly?
- Is the meter blocked?

If you cannot find a solution ask your supplier for technical support.

Permissible range vs. viscosity

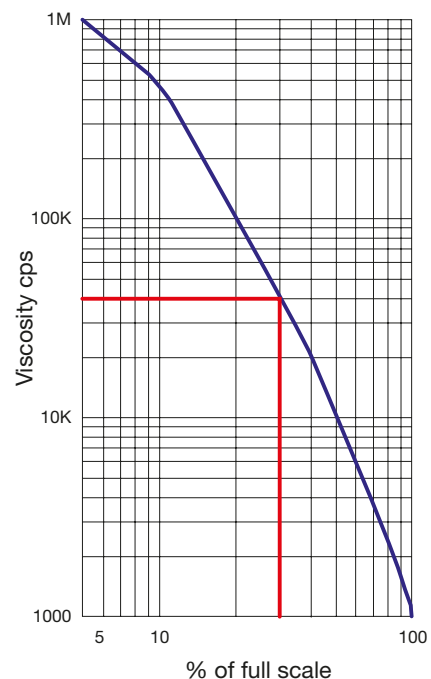

E.g. A 50 L/min. flowmeter measuring 40,000 cps would have a maximum flow range of 30% of full scale i.e. 15 L/min. All meters working above 1000 cps must have specially profiled gears.


# Oval Gear Flowmeter



Distributor: DDM GmbH & Co. KG

Phone: +49 661 967 962-0 >>> Email: [info@ddm-sensors.de](mailto:info@ddm-sensors.de) >>> Web: [www.ddm-sensors.de](http://www.ddm-sensors.de)

## STANDARD OVAL GEAR ASSEMBLY

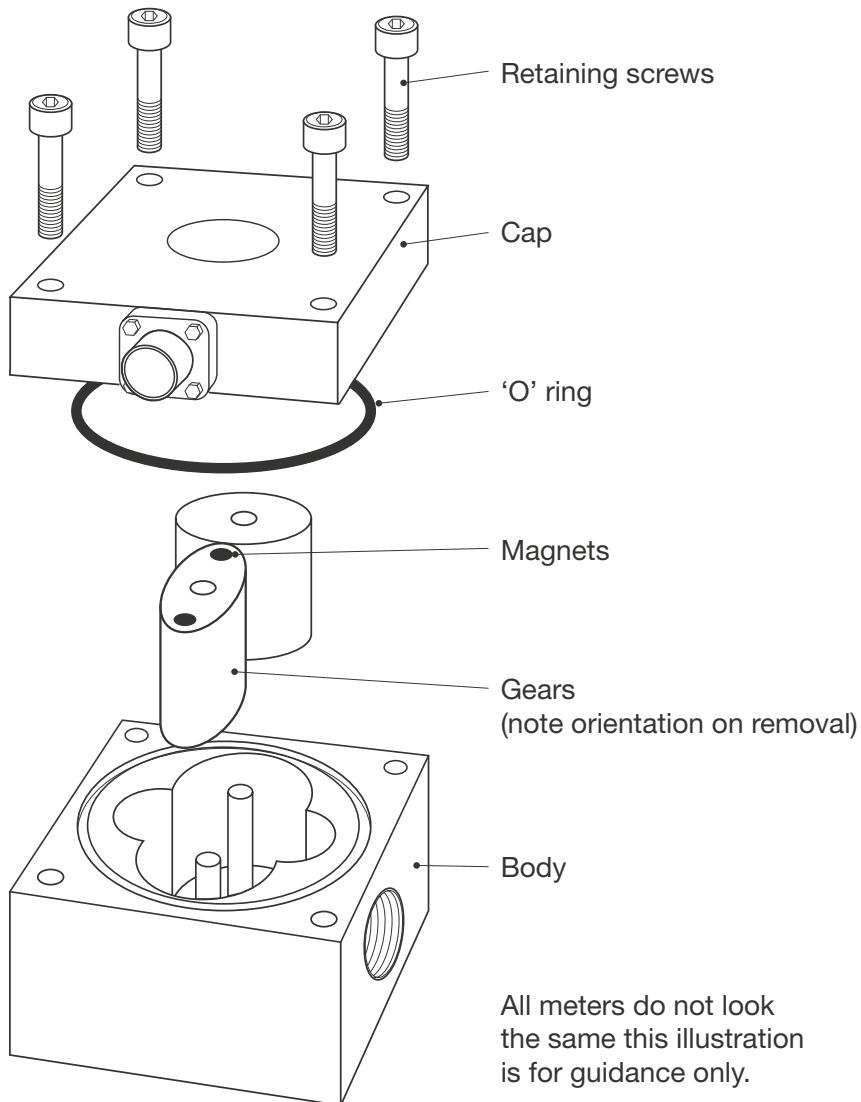

**TITAN ENTERPRISES LTD.**  
**Coldharbour Business Park, Sherborne, Dorset DT9 4JW**  
Tel: **(44) 01935 812790**  
Email: [sales@flowmeters.co.uk](mailto:sales@flowmeters.co.uk)  
[www.flowmeters.co.uk](http://www.flowmeters.co.uk)

*For reference only; for latest information contact your local distributor.*